

Type: KW4405

Serial no: 399

Sensitivity: 48.35 mV/Pa
-26.31 ±0.12 dB re. 1 V/Pa

Date: 6/7/2013

Signature: MB

Measurement conditions:


Polarisation voltage: 0.0 V
Pressure: 98.89 ±0.00 kPa
Temperature: 24.4 ±1.0 °C
Relative humidity: 59.7 ±2.0 %RH

Results are normalized to the reference conditions.

Free field response
Actuator response

Scantek, Inc.

6430 Dobbin Rd., Suite C, Columbia, MD 21045
Ph: 410-290-7726 eMail: callab@scantekinc.com

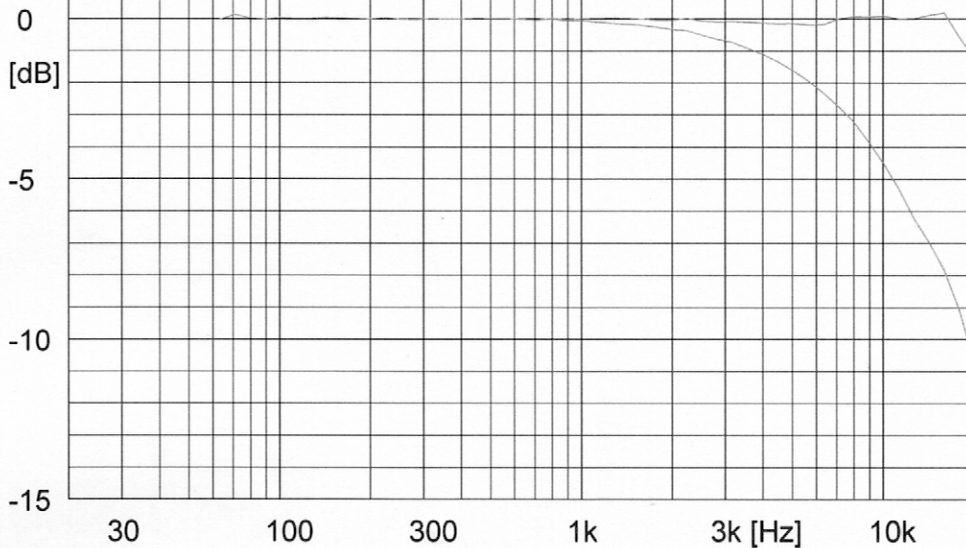

Microphone Test Report No.:28638

Audio Control
Type: KW4405

Serial no: 399

Sensitivity: 48.35 mV/Pa
-26.31 ±0.12 dB re. 1 V/Pa

Date: 6/7/2013

Signature: MB

Measurement conditions:


Polarisation voltage: 0.0 V
Pressure: 98.89 ±0.00 kPa
Temperature: 24.4 ±1.0 °C
Relative humidity: 59.7 ±2.0 %RH

Results are normalized to the reference conditions.

Free field response
Actuator response

Scantek, Inc.

6430 Dobbin Rd., Suite C, Columbia, MD 21045
Ph: 410-290-7726 eMail: callab@scantekinc.com

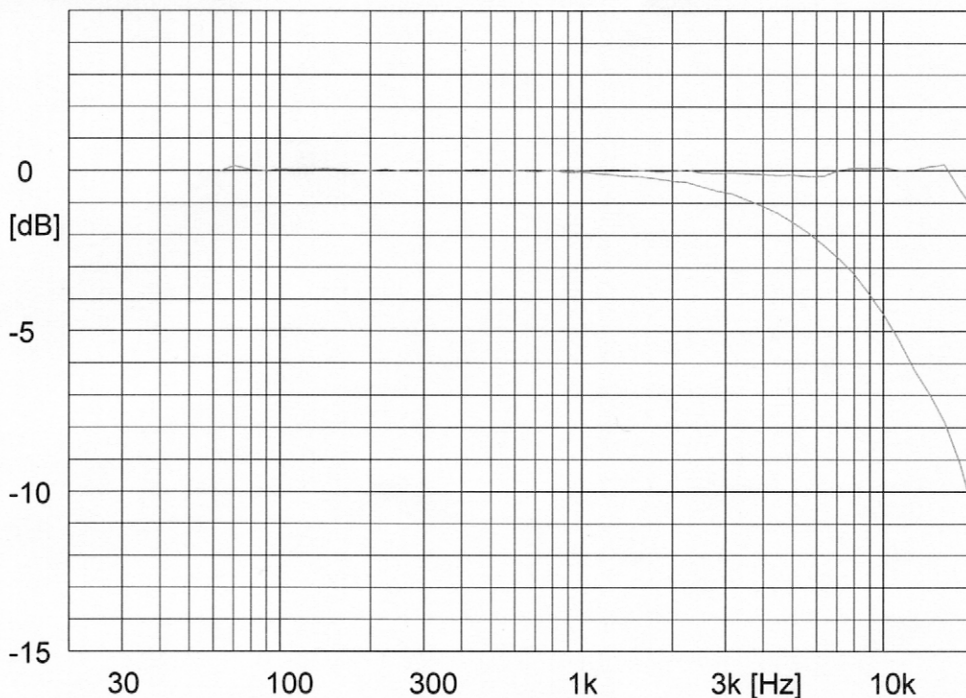

Comment: